International Journal of Engineering & Technology, 7 (4) (2018) 5460-5466

International Journal of Engineering & Technology

Website: www.sciencepubco.com/index.php/IJET
doi: 10.14419/ijet.v7i4.26056
Research paper

Testing and manufacturing with numerical modeling of metal PTB orthosis

Saif M. Abbas [1] *, Rasha Qasim Humadi [2], Ayad M. Takhakh [3]

[1] Al-Nahrain University, College of Engineering, Prosthetics and Orthotics Engineering Department, Baghdad, Iraq
[2] Advanced manufacturing Engineering, Baghdad, Iraq
[3] Al-Nahrain University, College of Engineering, Mechanical Engineering Department, Baghdad, Iraq
**Corresponding author E-mail: ayadtakak@yahoo.com*

Abstract

In this work, fiber glass as a reinforcement in composite material used for manufacturing ankle foot orthoses (AFO) PTB type of metal valve with vacuum molding technique fabricated. The material was depended on 8 layers of fiber glass. The mechanical properties of the AFOs' material were studied by tensile test, and fatigue test. The results showed that the tensile strength (σult) for fiber glass are 224 MPa, yield strength (σy) was 170 MPa and elongation at break 1.9mm.The gait cycle (ground reaction force (GRF)) and pressure distribution data were collected by using force plate and F-socket devices respectively for patient of age 29 years with height 185cm and weight 83kg .Heel contact time percent without PTBO equal to 5%, when wearing fiber glass PTBO equal to 59%. The midstance time percent for patient without PTBO equal to 12% when wearing PTBO equal to 34%. Solid work software program was used for PTPO modeling Also; the FEM (ANSYS ver.18.2) was used to compute the equivalent stress (Von-Mises), safety factor of fatigue and total deformation for fiber glass PTBO model. The obtained results from ANSYS gave the profile of safety factor of fatigue (1.1492).

Keywords: *Patellar Tendon-Bearing (PTB) Tensile; Fatigue; Fiber Glass; Modeling; Gait Analysis.*

1. Introduction

Orthoses are external appliances used to intercept or facilitate movement by supporting, aligning and Keep body parts. Orthotics can enhance the duty of dynamic body parts and prevent or correct deformation Orthoses can serve multiple functions, including controlling, correcting, facilitating, limiting, or inhibiting motion of the extremities or spine. Orthoses can also substitute for weak or paralyzed muscles and reduce muscle spasticity. These goals are not mutually exclusive; to maximize patient outcome, many clinical scenarios require complementary use of these functions. [1].
The PTBO was basically designed to support or off-load body weight for the below-knee part which is structurally inappropriate or causes pain fig show PTB orthosis [2]
In general the PTBOs part are manufactured usually of composite materials, due to their high strength to weight ratio specification, [3-4], therefore, the composite materials are modified through the years by adding of different components, variable number of laminated layers, [5-9]
H. Tanaka et. al, [10], estimated the unloading case effects of the patellar tendon-bearing (PTB) model for five healthy peoples using a dynamic plantar pressure system analysis. A method to enhance the unloading effect of the PTB, and tested this by using the same system. He concluded that the conventional PTB offers unloading of 30% of the body-weight while the part of the cast on the leg offered the most importance role in the unloading. It was also shown that when the depth of the space under the foot inside the PTB cast 1, 2 and 3 cm, the unloading effects were 60%, 80% and 98%, respectively.
The orthosis part investigation by many researcher with various parameters study, which investigation who to modifying the mechanical characterizations for its part, [11-20], or who to modifying the mechanical properties for materials using to manufacturing the orthosis part, [21-24]. Therefore, the best materials used to manufacturing the orthosis part is the composite materials, there, was to necessary the investigation of the composite materials properties and who can modified its properties and application for its materials. Then, various researchers studied the modifying ways of composite materials properties, [25-31], and different application for its materials, [32-40].
A wide range of materials are used in fabricating an orthosis and are frequently used in combination such as metals (are durable but are often considered unattractive and heavy), plastic (thermoplastic, thermoset….etc.) and fiber (fiber glass, carbon fiber…etc.) in this research a fiber glass has been used in the manufacturing of patellar tendon-bearing orthotic.

2. Experimental work

The experimental part is necessary work for engineering problem, which part given a good results of mechanical characterizations for its problem, which can be dependent on to investigation the behavior for its part, [41-43]. There, the experimental work including investigation for mechanical properties and characterizations for PTB orthosis part under various load condition. Therefore, its parts included manufacturing and testing of the composite materials using for orthsis part. Then, the following steps shown its steeping for manufacturing and testing materials orthsis part,

2.1. Materials

Copyright © 2018 Saif M. Abbas et al. This is an open access article distributed under the Creative Commons Attribution License, which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.

The materials of the PTBO needed in lamination for this study are as follows [44],

- Fiber glass and Lamination resins 80:20 polyurethane.
- Hardening powder.
- Polyvinyalcohol PVA bag.
- Materials for Jepson.

2.2. Preparing of samples for tensile, and fatigue tests

The preparing of samples for tensile and fatigue test, are as follows: Firstly Set the rectangular mold at the stand of vacuum pressure system. And Use the fiber glass stockinet as indicated by the overlaying lay-up. then Blend the overlay resin 80:20 polyurethane with the hardener. After that Maintain constant vacuum with pressure approximately (30-60 KPa) at room temperature. Until the laminations become cold cut according to the dimension of samples.

For tensile test three samples, [45-51], were prepared for lamination according to ASTM D638 type I. Fig. 1. shows the dimensions of tensile sample. Also, to evaluating the fatigue characterizations eight specimens are used, [52-55]. The dimensions of samples are length 100 mm and width 10 mm according to the fatigue device test while thickness various with the kinds of laminate, as shown in Fig.2.

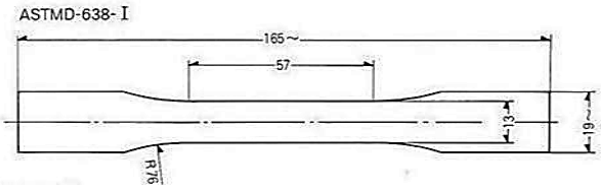


Fig. 1: The Dimensions of Tensile Sample According to ASTM D638.

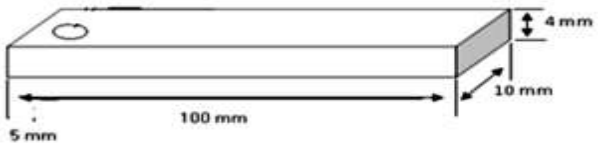


Fig. 2: Dimensions of Fatigue Samples.

2.3. Manufacturing procedure

The procedure of manufacturing metal PTB orthotic can be summarized as follows:

- Mounting the positive mold at the laminating stand.
- Putting the (8 fiber glass) layers and pulls the outer (PVA) bag.
- Mixing the Orthocryl lamination resin with the hardener about (800-900) ml of resin mixed with (2-3) part of hardener. The resulting matrix mixture is distributed homogenously inside the outside PVA bag.
- Maintaining constant vacuum and cut the resulting lamination in the shape of PTBO with required dimensions then placing Velcro closures with locating the place of the knee.
- Placing the side bars :The metal design consists of a metal structure shaped to the limb and upholstered with leather at the points where the device makes contact with a person's body, This orthosis consists of a rigid femoral stem and a calf foot part made of polyethylene or polypropylene, in some cases, leather can be used, A joint - locked or not - connects the two parts together, depending on the case, double-sided or single-sided high-rise, It is held with Velcro closures and the shoe, The most important step in this kind of orthosis is locating the place of the knee and determine Horizontal axis of the knee joint, Then modify the columns by meanders leg.
- Refining the trim lines and placing tapes: after cutting the shape of the orthosis, start to refine the edges and trim lines, placing the tapes on at the whole orthosis on the thigh area and calf and the foot.
- Alignment and Biomechanics: The alignment of the PTB orthosis is on the Adjust the horizontal axis of the ankle joint, let the patient wear it and walk with it and recognize the fixation of the deformity. Fig.3 shows the metal PTBO.

Then, testing patellar tendon-bearing by using the F-socket and gait cycle. Where, the Interface pressure test for patient wearing a metal PTB orthosis with age (29 years), height (185 cm) and weight (83 kg) suffered from left pain in the ankle and foot using sensor type (Mat Scan) which is acceptable for this type of dynamic load, as shown in Fig. 4.



Fig. 3: Metal PTB Orthosis.

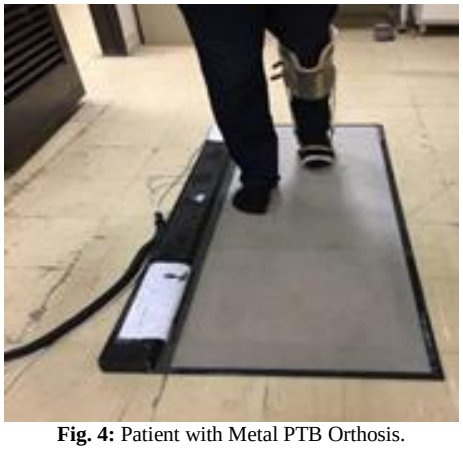


Fig. 4: Patient with Metal PTB Orthosis.

3. Numerical analysis

The PTB orthotic is drawing by using 3D SOLIDWORKS (version 2014) as shown in Fig. 5. SOLIDWORKS is a 3D mechanical CAD (computer aided design) program. ANSYS Workbench 18.2 software has been used as a numerical tool to illustrate the effect of the stress performance in a structure element. The analysis of PTBO's models for patient was established by FEM software to compute the equivalent (Von-Mises) stress, total deformation and safety factor of fatigue. According to the Von-Mises theory that considers the yield stress as criteria; ($\sigma e < \sigma y$, safe), ($\sigma e = \sigma y$, critical) and ($\sigma e > \sigma y$, failed). Where, (σe) is the equivalent stress, and (σy) is the yield stress. It is seen that the fatigue safety factor is safe in design applications if the safety factor is about or more than (1.25), [56-57].

Therefore, the numerical technique used to evaluated the mechanical characterizations for structure with various geometry and applied load conditions, [58-65]. In addition, the results for its technique can be depending to comparison with other techniques used, [66-74], to given the agreement for results were evaluated by analytical or experimental work.



Fig. 5: 3-D Modeling of the Metal PTB

4. Results and discussion

4.1. Tensile properties results

The mechanical properties of eight layers glass fiber with orthocryl lamination resin are listed in Table 1. Fig. 6 showed the stress-strain curve of fiber glass. Table 1 showed that there are large differences in the values of ultimate stresses, yield stress and modulus of elasticity between the glass fiber composite and polypropylene plastic materials, which were increased by more than 446%, 640% and 141% respectively as compared with Polypropylene.

Table 1: Mechanical Properties of Composite Material PTBO

PTBO Material	Thickness (mm)	Σy (MPa)	Σult (MPa)	E (GPa)
Composite fiber glass (8layers)	4.2	170	224	2.17
Polypropylene, [75]	4	23	28-41	0.9

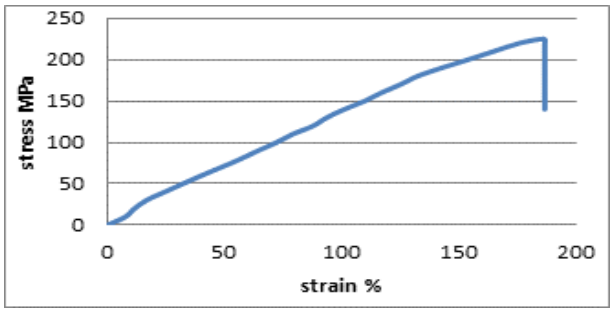


Fig. 6: Stress-Strain Curve for One Sample of Reinforced Composite with Fiber.

4.2. Fatigue test results

The result of fatigue test is shown in Fig. (7) show S-N curve for samples of lamination. The failure of fatigue of flat specimen can be occur when the specimen is fractured under periodic loading. The readings recorded by the fatigue tester machine, gave the number of cycles when the specimens were fractured. The failure stresses are decreasing and the numbers of cycles to reach to the failure are increasing at constant temperature.

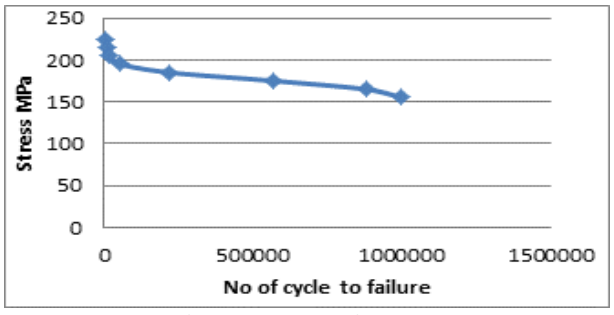


Fig. 7: S-N Curve for Composite Reinforcement with Fiber Glass.

4.3. Gait analysis with PTBO results

The ground reaction force (GRF) introduced under sole, due to biomechanical effects on leg during gait and stance cases walk over fixed plate where the force distribution is developed under sole due to patient gait. The test includes walking two main parts: before and after wearing PTB Orthosis . Fig.(8) shows the patients walking on force plate device with and without PTBO



Fig. 8: The Patient with and without PTBO.

a) Gait analysis without PTBO

Gait and gait cycle tables for patient without wearing PTBO results were shown in Tables 2 and 3 respectively. The main parameters describes the behavior of the gait cycle for patient separately as average data for one complete gait cycle from heel to heel strike. The force and the pressure distribution developed under sole due to patient gait for two feet are shown in Fig. (9), (10) restrictively.

Table 2: Gait Table for Patient without PTBO

gait table	patient without PTBO
Number of strikes	12
Cadence (steps/min)	47.6
gait time (sec)	10.08
Gait distance (cm)	368.9
Gait velocity (cm/sec)	36.6

Table 3: Gait Cycle without PTBO

gait cycle(sec)	patient without PTBO		
	Left	Right	difference
gait cycle time	2.06	2.98	0.93
Stance time	1.59	1.8	0.21
Initial double support time	0.50	0.42	-0.08
terminal double support time	0.42	0.50	0.08
total double support time	0.91	0.91	0.00
Heel contact time	1.12	1.17	0.05
Mid stance time	0.70	0.59	-0.12

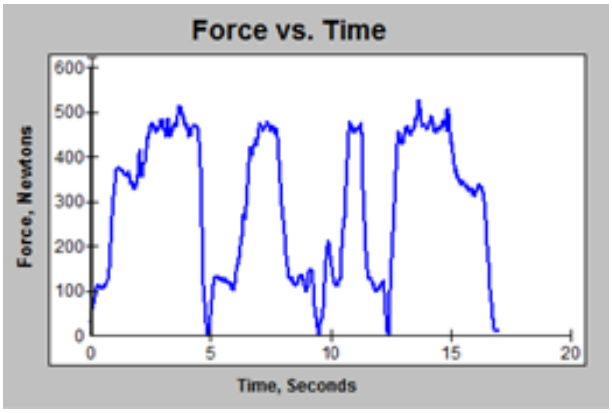


Fig. 9: Force vs. Time without PTBO.

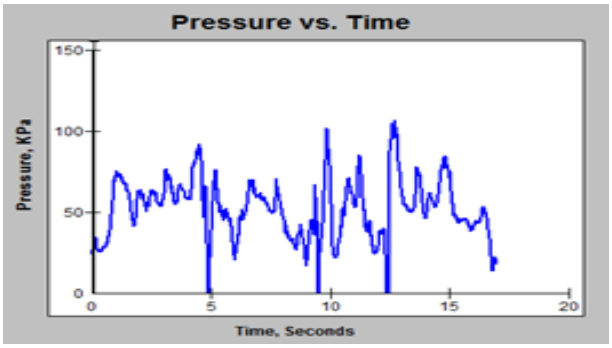


Fig. 10: Pressure vs. Time without PTBO.

b) 4.5. Gait analysis with metal PTBO

The main parameters describe the behavior of the gait cycle for patient wearing Metal PTBO separately as average data for one complete gait cycle from heel to heel strike. The results of the right were different from the left foot of the patient. Gait table and gait cycle table for patient with PTBO results were shown in Tables 4 and 5 respectively. The force and the pressure distribution developed under sole due to patient gait for two feet are shown in Fig. (11), (12) restrictively.

Table 4: Gait Table for Patient with PTBO

gait table	patient with PTBO
Number of strikes	11
Cadence (steps/min)	37
gait time (sec)	11.34
Gait distance (cm)	240.7
Gait velocity(cm/sec)	21.2

Table 5: Gait Table for Patient with PTBO

gait cycle	patient with PTBO		
	Left	Right	difference
gait cycle time	1.87	2.01	-0.14
Stance time	1.22	1.53	0.31
Initial double support time	0.1	0.22	0.13
terminal double support time	0.22	0.1	-0.13
total double support time	0.32	0.32	0.00
Heel contact time	0.38	0.97	0.59
Midstance time	0.94	0.61	-0.34

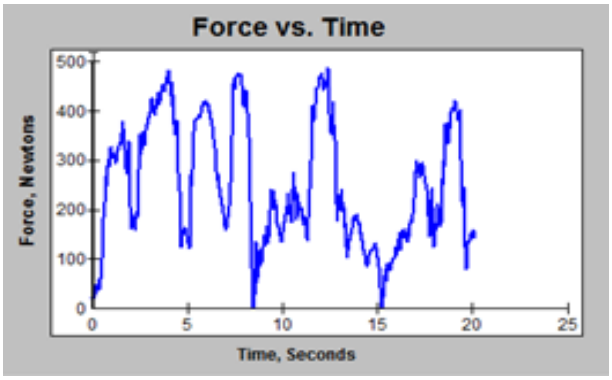


Fig. 11: force vs. Time with PTBO.

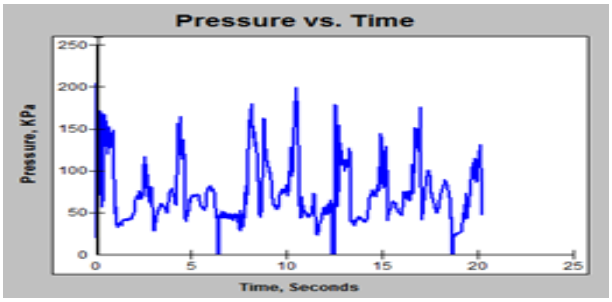


Fig. 12: Pressure vs. Time with PTBO.


The pressure distribution shows that at 50% of gait cycle the pressure reaches the maximum value because the ground reaction force is at maximum value in mid stance. The value of force with PTB Orthosis was 21.4 KN and the value of pressure with orthosis is 110 KPa that leads to better correction. The following result was obtained after achieving Gait cycle Test by using Force Plate device to determine the Ground reaction force GRF and interface pressure between the orthotics and the feet as shown in table 6.

From the comparison result obtained for the patient, as shown in the tables. The difference detected in the heel contact time and midstance time. heel contact time percent without PTBO equal to 5%, when wearing fiber glass PTBO equal to 59%. The midstance time percent for patient without PTBO equal to 12% when wearing PTBO equal to 34%. Reduction in the forces applied on foot after wearing orthotics and that is the main aim. the normal value of foot angle in men is 7 degrees and according to the above table it turns out that the angles of feet after wearing orthotics are increased and tend to be more normal so that's a good indication about orthotics well performance as shown in Fig. (13).

Table 6: Step Stride Comparison for the Case Study

Step Stride Table	Case study Without PTB		Case study With PTB	
Step Stride Table	right	left	right	Left
Step time (sec)	1.36	1.17	1.60	0.62
Step length(cm)	48.2	44	22.6	9
Step width(cm)	10.4	9.8	12.3	11.9
Step velocity (cm/sec)	35.8	37.6	14.1	14.5
Maximum force (N)	36.55	38.15	10.21	39.56
Maximum peak pressure (KPA)	236	206	172	225
Foot angle (degree)	0	2	-1	14

(A) Stance Time without PTBO

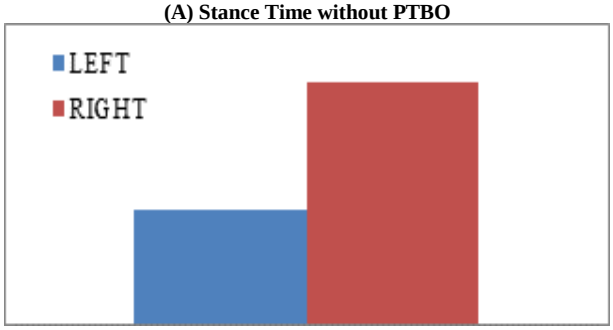

(B) Stance Time with PTBO

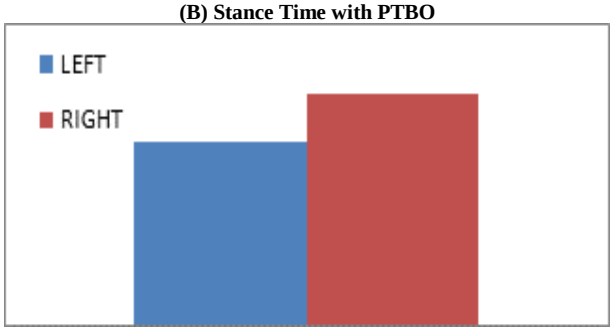


Fig. 13: Stance Time with and Without PTBO for Patient.

4.4. Interface pressure between the patient and PTBO

The alternating load between the calf and patient's leg, who was wearing the PTB, was measured as pressure. The sensor type (MatScan) is more acceptable for this type of dynamic load. The interface pressure was obtained by recording the output signal of the sensor through a multi-meter instrument which is interface with the computer and recording the data with the time. The pressures were only considered over the gait cycle by contact method between the patients and PTB at the calf reign. The data were normalized to 100 percent of gait cycle. The pressure for subjects was different at weight acceptance for as shown in Fig (14). The interface pressure between the stump of patient and socket can be measured using the F- Socket sensor. The sensor is driven by

computer software (F-Scan) in order to measure the applied pressure curve. The sensor was put on the lateral region of the stump and it turns out that higher pressure is 226 KPa.

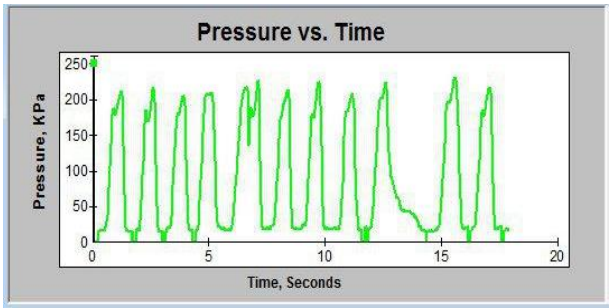


Fig. 14: Pressure vs. Time Percentage for Patient.

4.5. Numerical results

The analysis process and estimating of the Equivalent stresses, Total deformation and safety factor were done as shown below:

i) Equivalent stress (Von-Mises)

This stress is used to explain the fatigue S-N curve of the fatigue test taking into account the type of fatigue loading. Fig. (15) shows the overall distribution of the Von Mises stresses throughout the design and the approximate value and its location of the maximum Von Mises stress may be defined throughout the region of interest. The maximum stress was equal to 147.92 MPa.

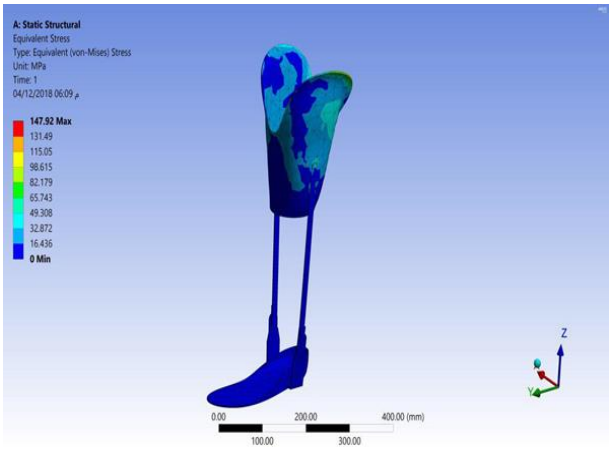


Fig. 15: Equivalent Stress (Von-Mises).

ii) Total deformation

Fig. (16) shows the maximum deformation for fiber glass lamination. The analysis process it has been found that the total deformation of Rigid Foot Orthosis is equal to 69.777 mm.

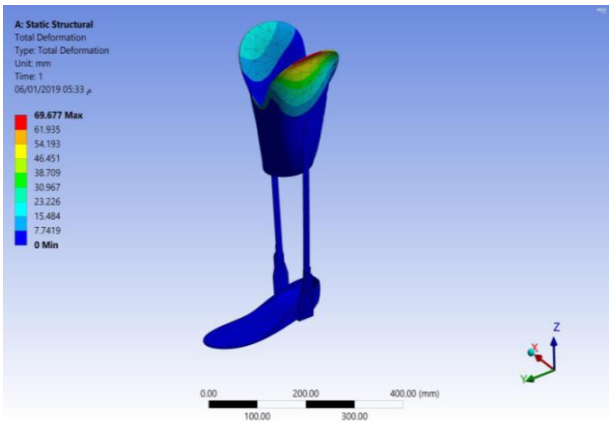


Fig. 16: Total Deformation.

iii) Safety Factor

The safety factor for polymer composite reinforced with fiber glass AFO model is passed in design as shown in the Fig. 17. The model of fiber glass material AFO showed that the fatigue safety factor for 8 layers of fiber glass is about (1.1492) which can be considered as safe as in design.

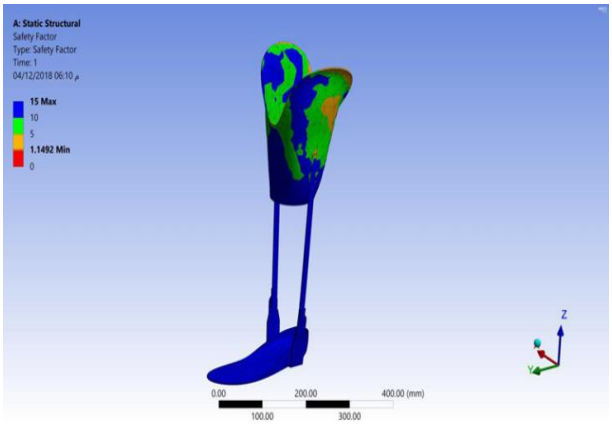


Fig. 17: The Safety Factor for Fatigue (Perlon).

5. Conclusion

This study gives a good database for manufacturing suitable lamination of an ankle foot ortheses suitable for patients. The conclusions of this work are as follows:

1) The results of the mechanical properties (σult, σy and E) showed that the KAFO made of 8 layers of glass fiber with orthocryl lamination resin were increased by 446%, 640% and 141% respectively as compared with that made of Polypropylene.
2) The model of material PTBO showed that the fatigue safety factor for (8 fiber glass) layers is equal to (1.1492) which is acceptable as safe as in design.
3) Maximum deformation is equal to 69.777 mm.
4) Higher interface pressure between the PTBO and patient is 226KPa at the calf region.

References

[1] Yasmeen A., Mohammed. The Role of New Technology in Designing and Fabrication of Orthosis and Prosthesis. M.Sc. Thesis, Zagazig University, 2008.

[2] [Khaira H. S., Coddington, A. Drew, P. N. Roberts and C. H. E. Imray. Patellar Tendon Bearing Orthosis - Application as Adjunctive Treatment in Healing of Lower-limb Tissue Loss. Eur J Vasc Endovasc Surg 16, 485488, 1998].

[3] Muhsin J. Jweeg, Ayad M. Takhakh, and Saif M. Abbas, Characterization of materials used in manufacturing the ankle foot ortheses , International Journal of Energy and Environment Issue on Applied Mechanics Research" Volume 8, Issue 4, pp.291298. (2017).

[4] Saif M. Abbas, Ayad M. Takhakh, Mohsin Abdullah Al-Shammari, Muhannad Al-Waily 'Manufacturing and Analysis of Ankle Disarticulation Prosthetic Socket (SYMES)' International Journal of Mechanical Engineering and Technology (IJMET), Vol. 09, No. 07, pp. 560-569, 2018.

[5] Ayad M. Takhakh, Saif M. Abbas 'Manufacturing and Analysis of Carbon Fiber Knee Ankle Foot Orthosis' International Journal of Engineering & Technology, Vol. 07, No. 04, pp. 2236-2240, 2018. https://doi.org/10.14419/ijet.v7i4.17315.

[6] S. M. Abbas 'Effects of Composite Material Layers on the Mechanical Properties for Partial Foot Prosthetic Socket' Al-Nahrain Journal for Engineering Sciences (NJES), Vol. 21, No. 02, pp. 253-258. (2018) https://doi.org/10.29194/NJES21020253.

[7] Saif M. Abbas, Kadhim K. Resan, Ahmed K. Muhammad, Muhannad Al-Waily 'Mechanical and Fatigue Behaviors of Prosthetic for Partial Foot Amputation with Various Composite Materials Types Effect' International Journal of Mechanical Engineering and Technology (IJMET), Vol. 09, No. 09, pp. 383–394, 2018.

[8] Ayad M. Takhakh, Saif M.Abbas, Aseel.K. Ahmed 'A Study of the Mechanical Properties and Gait Cycle Parameter for a Below-Knee

Prosthetic Socket' IOP Conference Series: Materials Science and Engineering, 2nd International Conference on Engineering Sciences, Vol. 433, 2018.
[9] Saif M. Abbas and Mohammed H Abbas " Analysis and manufacturing of above knee prosthesis socket by using revo fit solution" IOP Conf. Series: Materials Science and Engineering 454 (2018) 012025.
[10] H. Tanaka, K. Nagata, T. Goto, H. Hoshiko, A. Inoue. The effect of the patellar tendon-bearing cast on loading. J. of Bone and Joint Surgery [Br] 2000;82-B:228-32. https://doi.org/10.1302/0301-620X.82B2.0820228.
[11] Muhsin J. Jweeg, Sameer Hashim Ameen 'Experimental and theoretical investigations of dorsiflexion angle and life of an ankle-Foot-Orthosis made from (Perlon-carbon fibre-acrylic) and polypropylene materials' 10th IMEKO TC15 Youth Symposium on Experimental Solid Mechanics, 2011.
[12] Bashar A. Bedaiwi, Jumaa S. Chiad 'Vibration analysis and measurement in the below knee prosthetic limb part I: Experimental work' ASME 2012 International Mechanical Engineering Congress and Exposition, Proceedings (IMECE), 2012.
[13] Ayad M. Takhakh, Fahad M. Kadhim, Jumaa S. Chiad 'Vibration Analysis and Measurement in Knee Ankle Foot Orthosis for Both Metal and Plastic KAFO Type' ASME 2013 International Mechanical Engineering Congress and Exposition IMECE2013, November 15-21, San Diego, California, USA, 2013.
[14] Muhsin J. Jweeg, A. A. Alhumandy, H. A. Hamzah 'Material Characterization and Stress Analysis of Openings in Syme's Prosthetics' International Journal of Mechanical & Mechatronics Engineering IJMME-IJENS, Vol. 17, No. 04, 2017.
[15] Zainab Yousif Hussien, Kadhim Kamil Resan 'Effects of Ultraviolet Radiation with and without Heat, on the Fatigue Behavior of Below-Knee Prosthetic Sockets' International Journal of Mechanical and Production Engineering Research and Development (IJMPERD), Vol. 07 , No. 06, 2017.
[16] Mahmud Rasheed Ismail, Muhannad Al-Waily, Ameer A. Kadhim 'Biomechanical Analysis and Gait Assessment for Normal and Braced Legs' International Journal of Mechanical & Mechatronics Engineering IJMME-IJENS, Vol. 18, No. 03, 2018.
[17] Fahad M Kadhim, Jumaa S Chiad, Ayad M Takhakh 'Design And Manufacturing Knee Joint for Smart Transfemoral Prosthetic' IOP Conference Series: Materials Science and Engineering, International Conference on Materials Engineering and Science, Vol. 454, 2018.
[18] Noor Dhia Yaseen, Jumaa S. Chiad, Firas Mohammed Abdul Ghani 'The Study and Analysis of Stress Distribution Subjected on the Replacement Knee Joint Components using Photo-Elasticity and Numerical Methods' International Journal of Mechanical and Production Engineering Research and Development (IJMPERD), Vol. 08, No. 06, pp. 449-464, 2018. https://doi.org/10.24247/ijmperddec201849.
[19] Muhsin J. Jweeg, Zaid S. Hammoudi, Bassam A. Alwan 'Optimised Analysis, Design, and Fabrication of Trans-Tibial Prosthetic Sockets' IOP Conference Series: Materials Science and Engineering, 2nd International Conference on Engineering Sciences, Vol. 433, 2018.
[20] Muhsin J. Jweeg, Muhannad Al-Waily, Ahmed K. Muhammad, Kadhim K. Resan 'Effects of Temperature on the Characterisation of a New Design for a Non-Articulated Prosthetic Foot' IOP Conference Series: Materials Science and Engineering, Vol. 433, 2nd International Conference on Engineering Sciences, Kerbala, Iraq, 26–27 March, 2018. https://doi.org/10.1088/1757-899X/433/1/012064.
[21] Muhsin J. Jweeg, Kadhim K. Resan, Mustafa Tariq Ismail 'Study of Creep-Fatigue Interaction in a Prosthetic Socket Below Knee' ASME International Mechanical Engineering Congress and Exposition, 2012. https://doi.org/10.1115/IMECE2012-85240.
[22] Mohsin Abdullah Al-Shammari, Emad Q. Hussein, Ameer Alaa Oleiwi 'Material Characterization and Stress Analysis of a Through Knee Prosthesis Sockets' International Journal of Mechanical & Mechatronics Engineering IJMME-IJENS, Vol. 17, No. 06, 2017.
[23] Ahmed Khaleel Abdulameer, Mohsin Abdullah Al-Shammari 'Fatigue Analysis of Syme's Prosthesis' International Review of Mechanical Engineering, Vol. 12, No. 03, 2018. https://doi.org/10.15866/ireme.v12i3.14390.
[24] Ayad M. Takhakh 'Manufacturing and Analysis of Partial Foot Prosthetic for The Pirogoff Amputation' International Journal of Mechanical & Mechatronics Engineering IJMME-IJENS, Vol. 18, No. 03, pp. 62-68, 2018.
[25] Muhsin J. Jweeg, Ali S. Hammood, Muhannad Al-Waily 'Experimental and Theoretical Studies of Mechanical Properties for Reinforcement Fiber Types of Composite Materials' International Journal of Mechanical & Mechatronics Engineering IJMME-IJENS, Vol. 12, No. 04, 2012.
[26] Muhannad Al-Waily, Zaman Abud Almalik Abud Ali 'A Suggested Analytical Solution of Powder Reinforcement Effect on Buckling Load for Isotropic Mat and Short Hyper Composite Materials Plate' International Journal of Mechanical & Mechatronics Engineering IJMME-IJENS, Vol. 15, No. 04, 2015.
[27] Abdulkareem Abdulrazzaq Alhumdany, Muhannad Al-Waily, Mohammed Hussein Kadhim Al-Jabery 'Theoretical and Experimental Investigation of Using Date Palm Nuts Powder into Mechanical Properties and Fundamental Natural Frequencies of Hyper Composite Plate' International Journal of Mechanical & Mechatronics Engineering IJMME-IJENS, Vol. 16, No. 01, 2016.
[28] Muhannad Al-Waily, Alaa Abdulzahra Deli, Aziz Darweesh Al-Mawash, Zaman Abud Almalik Abud Ali 'Effect of Natural Sisal Fiber Reinforcement on the Composite Plate Buckling Behavior' International Journal of Mechanical & Mechatronics Engineering IJMME-IJENS, Vol. 17, No. 01, 2017.
[29] Ahmed A. Taher, Ayad M. Takhakh, Sabah M. Thaha 'Experimental Study and Prediction the Mechanical Properties of Nano-Joining Composite Polymers' Journal of Engineering and Applied Sciences, Vol. 13, No. 18, pp. 7665, 7669, 2018.
[30] Mohsin Abdullah Al-Shammari, Sahar Emad Abdullah 'Stiffness to Weight Ratio of Various Mechanical and Thermal Loaded Hyper Composite Plate Structures' IOP Conference Series: Materials Science and Engineering, 2nd International Conference on Engineering Sciences, Vol. 433, 2018.
[31] Ameer A. Kadhim, Muhannad Al-Waily, Zaman Abud Almalik Abud Ali, Muhsin J. Jweeg, Kadhim K. Resan 'Improvement Fatigue Life and Strength of Isotropic Hyper Composite Materials by Reinforcement with Different Powder Materials' International Journal of Mechanical & Mechatronics Engineering IJMME-IJENS, Vol. 18, No. 02, 2018.
[32] Luay S. Al-Ansari, Muhannad Al-Waily, Ali M. H. Yusif 'Vibration Analysis of Hyper Composite Material Beam Utilizing Shear Deformation and Rotary Inertia Effects' International Journal of Mechanical & Mechatronics Engineering IJMME-IJENS, Vol. 12, No. 04, 2012.
[33] Muhsin J. Jweeg, Ali S. Hammood, Muhannad Al-Waily 'A Suggested Analytical Solution of Isotropic Composite Plate with Crack Effect' International Journal of Mechanical & Mechatronics Engineering IJMME-IJENS, Vol. 12, No. 05, 2012.
[34] Mohsin Abdullah Al-Shammari, Muhannad Al-Waily 'Theoretical and Numerical Vibration Investigation Study of Orthotropic Hyper Composite Plate Structure' International Journal of Mechanical & Mechatronics Engineering IJMME-IJENS, Vol. 14, No. 06, 2014.
[35] Jumaa S. Chiad 'Study the Impact Behavior of the Prosthetic Lower Limb Lamination Materials due to Low Velocity Impactor' ASME 2014 12th Biennial Conference on Engineering Systems Design and Analysis, ESDA, 2014, July 25–27, 2014.
[36] Muhsin J. Jweeg, Muhannad Al-Waily, Alaa Abdulzahra Deli 'Theoretical and Numerical Investigation of Buckling of Orthotropic Hyper Composite Plates' International Journal of Mechanical & Mechatronics Engineering IJMME-IJENS, Vol. 15, No. 04, 2015.
[37] Muhsin J. Jweeg 'A Suggested Analytical Solution for Vibration of Honeycombs Sandwich Combined Plate Structure' International Journal of Mechanical & Mechatronics Engineering IJMME-IJENS, Vol. 16, No. 02, 2016.
[38] Muhannad Al-Waily, Kadhim K. Resan, Ali Hammoudi Al-Wazir, Zaman Abud Almalik Abud Ali 'Influences of Glass and Carbon Powder Reinforcement on the Vibration Response and Characterization of an Isotropic Hyper Composite Materials Plate Structure' International Journal of Mechanical & Mechatronics Engineering IJMME-IJENS, Vol. 17, No. 06, 2017.
[39] Mohsin Abdullah Al-Shammari 'Experimental and FEA of the Crack Effects in a Vibrated Sandwich Plate' Journal of Engineering and Applied Sciences, Vol. 13, No. 17, pp. 7395-7400, 2018.
[40] Jumaa S. Chiad, Muhannad Al-Waily, Mohsin Abdullah Al-Shammari 'Buckling Investigation of Isotropic Composite Plate Reinforced by Different Types of Powders' International Journal of Mechanical Engineering and Technology (IJMET), Vol. 09, No. 09, pp. 305–317, 2018.
[41] Adnan S. Jabur, Jalal M. Jalil, Ayad M. Takhakh 'Experimental Investigation and Simulation of Al-Si Casting Microstructure Formation' Arabian Journal for Science and Engineering, Vol. 37, No. 03, pp. 777-792, 2012. https://doi.org/10.1007/s13369-012-0189-2.
[42] Ragad Aziz Neama, Maher A.R. Sadiq Al-Baghdadi, Muhannad Al-Waily 'Effect of Blank Holder Force and Punch Number on the Forming Behavior of Conventional Dies' International Journal of

Mechanical & Mechatronics Engineering IJMME-IJENS, Vol. 18, No. 04, 2018.
[43] H. J. Abbas, M. J. Jweeg, Muhannad Al-Waily, Abbas Ali Diwan 'Experimental Testing and Theoretical Prediction of Fiber Optical Cable for Fault Detection and Identification' Journal of Engineering and Applied Sciences, Vol. 14, No. 02, pp. 430-438, 2019.
[44] Ottobock QWuality for Life "Orthotic- Prosthetic Materials Cataloge",(2007).
[45] Ghaith G. Hameed, Muhsin J. Jweeg, Ali Hussein 'Springback and side wall curl of metal sheet in plain strain deep drawing' Research Journal of Applied Sciences, Vol. 04, No. 05, pp. 192-201, 2009.
[46] Ayad M. Takhakh, Raied Z. Alfay, Abdul Rahim K. Abid Ali 'Effect of Ta addition on hardness and wear resist of Cu-Al-Ni shape memory alloy fabricated by powder metallurgy' BEIAC 2013-2013 IEEE Business Engineering and Industrial Applications Colloquium, 2013.
[47] Muhsin J. Jweeg, E. Q. Hussein, K. I. Mohammed 'Effects of Cracks on the Frequency Response of a Simply Supported Pipe Conveying Fluid' International Journal of Mechanical & Mechatronics Engineering IJMME-IJENS, Vol. 17, 05, 2017.
[48] Muhsin J. Jweeg, Kadhim K. Resan, Esraa A. Abbod, Muhannad Al-Waily 'Dissimilar Aluminium Alloys Welding by Friction Stir Processing and Reverse Rotation Friction Stir Processing' IOP Conference Series: Materials Science and Engineering, Vol. 454, International Conference on Materials Engineering and Science, Istanbul, Turkey, 8 August, 2018. https://doi.org/10.1088/1757-899X/454/1/012059.
[49] Abeer R. Abbas, Kadhim A. Hebeatir, Kadhim K. Resan 'Effect of CO2 Laser on Some Properties of NI46TI50CU4 Shape Memory Alloy' International Journal of Mechanical and Production Engineering Research and Development, Vol. 08, No. 02, pp. 451-460, 2018. https://doi.org/10.24247/ijmperdapr201852.
[50] Marwah Mohammed Abdulridha, Nasreen Dakel Fahad, Muhannad Al-Waily, Kadhim K. Resan 'Rubber Creep Behavior Investigation with Multi Wall Tube Carbon Nano Particle Material Effect' International Journal of Mechanical Engineering and Technology (IJMET), Vol. 09, No. 12, pp. 729-746, 2018.
[51] Abeer R. Abbas, Kadhim A. Hebeatir, Kadhim K. Resan 'Effect of Laser Energy on the Structure of Ni46–Ti50–Cu4 Shape-Memory Alloy' International Journal of Nanoelectronics and Materials, Vol. 11, No. 04, pp. 481-498, 2018.
[52] A. R. I. Kheder, N. M. Jubeh, E. M. Tahah 'Fatigue behavior of alloyed acicular ductile iron' International Journal for the Joining of Materials, Vol. 17, No. 01, pp. 7-12, 2005.
[53] A. R. I. Kheder, N. M. Jubeh, E. M. Tahah 'Fatigue properties under constant stress/variable stress amplitude and coaxing effect of acicular ductile iron and 42 CrMo4 steel' Jordan Journal of Mechanical and Industrial Engineering, Vol. 05, No. 04, 2011.
[54] Worood Hussein, Mohsin Abdullah Al-Shammari 'Fatigue and Fracture Behaviours of FSW and FSP Joints of AA5083-H111 Aluminium Alloy' IOP Conference Series: Materials Science and Engineering, International Conference on Materials Engineering and Science, Vol. 454, 2018. https://doi.org/10.1088/1757-899X/454/1/012055.
[55] Kadhim K. Resan, Abbas A. Alasadi, Muhannad Al-Waily, Muhsin J. Jweeg 'Influence of Temperature on Fatigue Life for Friction Stir Welding of Aluminum Alloy Materials' International Journal of Mechanical & Mechatronics Engineering IJMME-IJENS, Vol. 18, No. 02, 2018.
[56] Muhsin J. Jweeg, Ayad M. Takhakh, and Saif M. Abbas, Characterization of materials used in manufacturing the ankle foot ortheses , International Journal of Energy and Environment Issue on Applied Mechanics Research" Volume 8, Issue 4, pp.291298. (2017)
[57] Brett A. Miller, "Failure Analysis and Prevention, Fatigue Failures", ASM International Handbook. Vol. 11, P 58. 2002.
[58] Muhsin J. Jweeg 'Application of finite element analysis to rotating fan impellers' Doctoral Thesis, Aston University, 1983.
[59] Najdat A. Mahmood, Muhsin J. Jweeg, Mumtaz Y. Rajab 'Investigation of partially pressurized thick cylindrical shells' Modelling, simulation & control. B. AMSE Press, Vol. 25, No. 03, pp. 47-64, 1989.
[60] Muhsin J. Jweeg, S. Z. Said 'Effect of rotational and geometric stiffness matrices on dynamic stresses and deformations of rotating blades' Journal of the Institution of Engineers (India): Mechanical Engineering Division, Vol. 76, pp. 29-38, 1995.
[61] Ahmed Hasson, Muhsin J. Jweeg 'Soil organic carbon sequestration under pastures in arid region' Nature Environment and Pollution Technology, Vol. 12, No. 01, pp. 57-62, 2013.
[62] Muhannad Al-Waily, Maher A.R. Sadiq Al-Baghdadi, Rasha Hayder Al-Khayat 'Flow Velocity and Crack Angle Effect on Vibration and Flow Characterization for Pipe Induce Vibration' International Journal of Mechanical & Mechatronics Engineering IJMME-IJENS, Vol. 17, No. 05, pp.19-27, 2017.
[63] Rasha Hayder Al-Khayat, Maher A. R. Sadiq Al-Baghdadi, Ragad Aziz Neama, Muhannad Al-Waily 'Optimization CFD Study of Erosion in 3D Elbow During Transportation of Crude Oil Contaminated with Sand Particles' International Journal of Engineering & Technology, Vol. 07, No. 03, pp. 1420-1428, 2018. https://doi.org/10.14419/ijet.v7i3.14180.
[64] Mohsin Abdullah Al-Shammari, Lutfi Y. Zedan, Akram M. Al-Shammari 'FE simulation of multi-stage cold forging process for metal shell of spark plug manufacturing' 1st International Scientific Conference of Engineering Sciences-3rd Scientific Conference of Engineering Science, ISCES 2018–Proceedings, 2018. https://doi.org/10.1109/ISCES.2018.8340555.
[65] Mahmud Rasheed Ismail, Zaman Abud Almalik Abud Ali, Muhannad Al-Waily 'Delamination Damage Effect on Buckling Behavior of Woven Reinforcement Composite Materials Plate' International Journal of Mechanical & Mechatronics Engineering IJMME-IJENS, Vol. 18, No. 05, pp. 83-93, 2018.
[66] Mohsin Abdullah Al-Shammari, Muhannad Al-Waily 'Analytical Investigation of Buckling Behavior of Honeycombs Sandwich Combined Plate Structure' International Journal of Mechanical and Production Engineering Research and Development (IJMPERD), Vol. 08, No. 04, pp. 771-786, 2018.
[67] Jumaa S. Chiad, Fadhel Abbas Abdulla 'Effect of Number and Location of Dampers on Suspension System for Washing Machine' International Journal of Mechanical Engineering and Technology (IJMET), Vol. 09, No. 08, pp. 794-804, 2018.
[68] Ehab N. Abbas, Muhsin J. Jweeg, Muhannad Al-Waily 'Analytical and Numerical Investigations for Dynamic Response of Composite Plates Under Various Dynamic Loading with the Influence of Carbon Multi-Wall Tube Nano Materials' International Journal of Mechanical & Mechatronics Engineering IJMME-IJENS, Vol. 18, No. 06, pp. 1-10, 2018.
[69] Maher A. R. Sadiq Al-Baghdadi 'A Simulation Model for a Single Cylinder Four-Stroke Spark Ignition Engine Fueled with Alternative Fuels' Turkish Journal of Engineering and Environmental Sciences, Vol. 30, pp. 331-350, 2006.
[70] Maher A.R. Sadiq Al-Baghdadi 'A CFD Study of Hygro-Thermal Stresses Distribution in PEM Fuel Cell During Regular Cell Operation' Renewable Energy Journal, Vol. 34, No. 03, pp.674-682, 2009. https://doi.org/10.1016/j.renene.2008.05.023.
[71] Maher A. R. Sadiq Al-Baghdadi 'A CFD Analysis of Transport Phenomena and Electrochemical Reactions in a Tubular-Shaped Ambient Air-Breathing PEM Micro Fuel Cell' HKIE Transactions Hong Kong Institution of Engineers, Vol. 17, No. 02, 2010.
[72] Bashar A. Bedaiwi 'Analyzing of Impact, Vibration Response and Stability of Artificial Upper Limb' American Society of Mechanical Engineering, ASME 2013 International Mechanical Engineering Congress and Exposition, Biomedical and Biotechnology Engineering, Vol. 3B, 2013.
[73] Sadeq H. Bakhy, Shaker S. Hassan, Somer M. Nacy, K. Dermitzakis, Alejandro Hernandez Arieta 'Contact Mechanics for soft Robotic Fingers: Modeling and Experimentation' Robotica, Vol. 31, No. 04, pp. 599-609, 2013. https://doi.org/10.1017/S0263574712000653.
[74] Jawad K. Oleiwi, Ahmed Namah Hadi 'Experimental and numerical investigation of lower limb prosthetic foot made from composite polymer blends' International Journal of Mechanical and Production Engineering Research and Development, Vol. 08, No. 02, pp. 1319-1330, 2018. https://doi.org/10.24247/ijmperdapr2018151.
[75] R.A. Flinn and Trojan PK 'Engineering Materials and Their Application' 4 thed Bostan, Houghton Mifflin, 1990.